



**Parts of the FALCON**

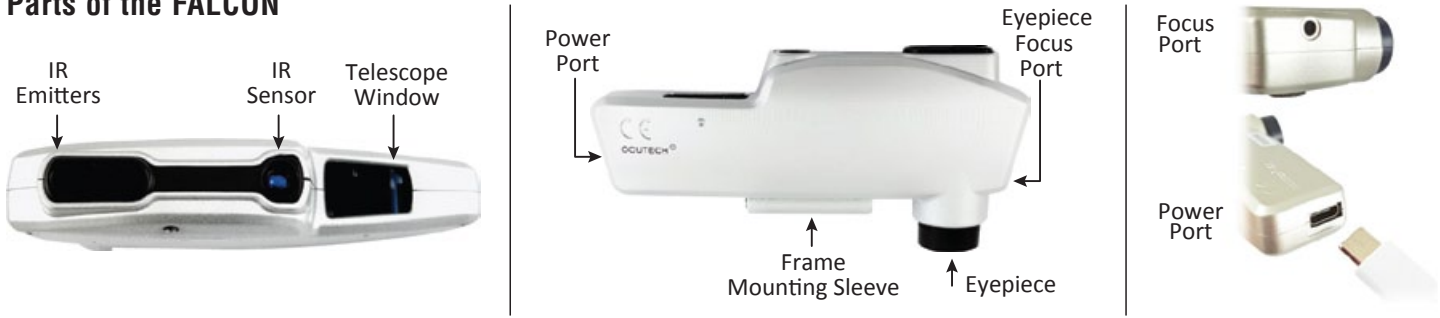

**1. Align the eyepiece to center above the patient's pupil.**

- a. Loosen the two bridge screws.
- b. Slide the telescope right or left to position the eyepiece directly above the pupil. Once in position retighten the bridge screws slightly, but do NOT over-tighten.
- c. **To switch the telescope from one eye to the other,** loosen the two rear bridge screws and slide the telescope off the positioning rod. Flip the telescope over and slide it back onto the rod, then re-tighten the screws to keep it in position. **Do NOT over-tighten the bridge screws.**

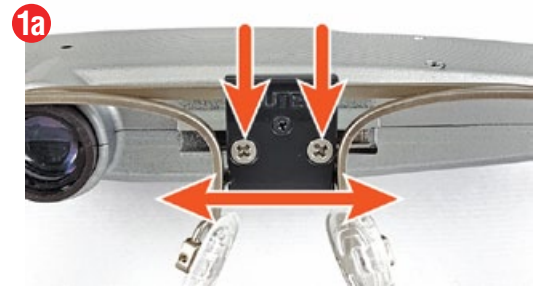

**2. Align the vertical position of the telescope eyepiece**

- a. Adjust the nosepads on the frame to align the bottom of the eyepiece with the top of the patient's pupil
- b. When looking below the Falcon, the telescope will have an upward tilted position. The red arrow shows angle of telescope while looking beneath the Falcon.
- c. Ask the patient to dip their head downward to look through the telescope eyepiece. Adjust the viewing angle tilt of the telescope to be parallel to the line of sight of the patient. The red arrow shows the straight-ahead position of the falcon



**3. Connect the USB cable to the battery**

- a. Do not disconnect the cable from the telescope itself.
- b. The battery will turn on automatically when the USB cable is connected. The Falcon will automatically run a brief self-check (this will occur every time the power is turned on). Press the power status button (red arrow) to confirm that the battery has adequate charge to operate the Falcon. The number of lights illuminated shows the percent of charge. The Falcon will operate for approximately 8 hours on a full battery charge.
- c. Recharge the battery using the Micro-USB cable provided.
- d. **To turn off the Falcon,** simply remove the USB cable from the battery.



USB-C cable connected to Falcon (do not remove)

Power supply cable

Battery charge cable

**4. Adjust the eyepiece focus**

Connect the Falcon to the battery and confirm that the motor is operating. The focus may not yet appear sharp to the patient.

- Instruct your patient to look through the Falcon eyepiece at a flat high contrast target more than 4 feet (1.2 m) away.
- Insert the eyepiece focus tool into the focus access port and rotate it to move the eyepiece in or out until the image is as sharp as possible for the patient. The eyepiece adjustment will cover refractive error from +/-8D. Refractions higher than 8D or 3D cyl may require eyepiece corrections. Consider using a contact lens when testing individuals with higher prescriptions.
- Carefully remove the eyepiece focus tool without rotating it.

**5. When dispensing the Falcon tighten the setscrew to fix eyepiece focus adjustment in place.**

BE CERTAIN TO LOOSEN THE SETSCREW BEFORE YOU READJUST THE EYEPIECE FOCUS

**6. When dispensing the Falcon to a patient insert the rubber plug to close the eyepiece focus access port.**

When inserting the plug into the access port the line on the head of the plug should be positioned horizontally.

**7. Using the Focus Override button**

On occasion the autofocus will not focus as the user might expect. This may occur when looking at an unusually reflective target or when looking through a window. By pressing the focus override button briefly (red arrow), the focus will hold at the distance it was focused. By pressing the button again, the autofocus will reactivate. By pressing the override button for several seconds, the Falcon will automatically shift focus to infinity and hold. By pressing the button again, the autofocus will reactivate.



- **Short Press:** the focus will hold at the current distance.
- **Long Press:** the focus will change to optical infinity.
- **Restart autofocusing:** pressing the button again will reactivate autofocusing.

**8. Use the head-strap to stabilize the Falcon on the head.**

The strap should be snug but NOT tight. DO NOT over-tighten the head-strap as this can reduce wearing comfort.

**9. Care and cleaning of the Falcon Autofocus Biopic**

- DO NOT IMMERSE THE FALCON IN WATER
- DO USE the provided lens cloth to keep the front window and eyepiece clean and free from fingerprints. You can lightly moisten the front window and the eyepiece lens with an approved lens cleaner and Q-tip and then dry with the lens cloth.
- DO NOT use abrasive cleaners on any part of the Falcon.
- DO NOT attempt to reposition the Falcon on the frame or the eyepiece without first loosening the frame or eyepiece set screws. An experienced individual should only perform this operation.
- DO NOT share the Falcon with another individual as the device has been carefully fitted and prescribed for the intended user.
- DO NOT leave the Falcon in a vehicle or other location where it can be exposed to high heat.
- DO NOT use the Falcon while driving unless properly trained and licensed.

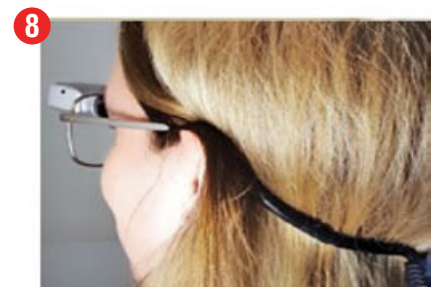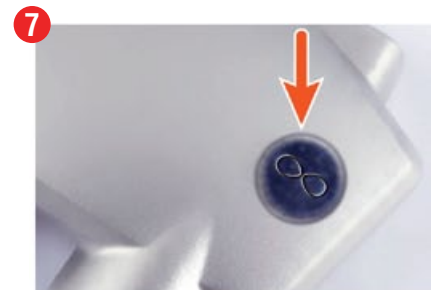

Warranty: The VES-Falcon is warranted against defects in parts and manufacture for 12 months from the date of shipping. Batteries and cables provided with the VES-Falcon are warranted for 90 days. There are no other warranties expressed or implied.

**ONLY use Ocutech approved batteries to operate your VES-Falcon.** Ocutech is not responsible for damage to your device if used with an unapproved battery.